

Indonesian Journal of Physical Education and Sport Science (IJPESS) Published By Universitas Nahdlatul Ulama Cirebon. This journal that focuses on Physical Education, Sports Science, Tourism Sports, Traditional Sports, Sports Biomechanics, Sport Health, Sports Nutrition, Sports Psychology and Sports Exercises. registered with LIPI and [BRIN](#) with [p-ISSN [2775-765x](#) | e-ISSN [2776-0200](#)]. IJPESS published the first edition in March 2021. IJPESS has been indexed by: [Sinta](#), [DOAJ](#), [SEAL](#), [EBSCO](#), [Copernicus](#), [Garuda](#), [Google Scholar](#), [Dimensions](#), [Crossref](#)

In 2024 the journal comes out every three months:

- March
- June
- September
- December

Manuscripts are submitted online.

Vol. 5 No. 3 (2025): September: Article in Progress

p-ISSN 2775-765X
e-ISSN 2776-0202

English

Bahasa Indonesia

SERTIFIKAT

Indonesian Journal of Psychology: Jurnal dan Studi tentang Psikologi
Indonesian Journal of Psychology: Jurnal dan Studi tentang Psikologi

Karya dan Riset dalam Bidang Psikologi, Tesis, dan Studi tentang Psikologi dan Psikologi, Jurnal dan Studi tentang Psikologi

Indonesian Journal of Psychology
Volume 1, Issue 1, 2015
Indonesian Journal of Psychology: Jurnal dan Studi tentang Psikologi

TERAKREDITASI

Indonesian Journal of Psychology: Jurnal dan Studi tentang Psikologi

Recommended Journal:

Journal Universitas Nahdlatul Ulama
Cirebon

Menu:

Editorial Team

Home / Editorial Team

Editorial Team

Editor in Chief:

Dr. Mikkey Anggara Suganda., M.Or. ID Scopus [58164051500](#) Universitas Nahdlatul Ulama Cirebon. Indonesia

Section Editor:

Indonesia

Risa Herdiyana Bastian., M.Pd. ID Scopus [59003373100](#), Universitas Nahdlatul Ulama Cirebon. Indonesia

Syifa Nurbait., M.Pd. D ID Scopus [59241944900](#) Universitas Nahdlatul Ulama Cirebon. Indonesia

Dr. Ardo Okilanda., M.Pd., ID Scopus [57224962924](#). Universitas Negeri Padang. Indonesia

Dr. Khairul Amar, M.Or., AIFO. ID Scopus [57217048198](#) STKIP Taman Siswa Bima. Indonesia

Internationals

Podrihalo Olha. ID Scopus [57219950990](#), Kharkiv State Academy of Physical Culture. Ukraina

Dr Hemantajit Gogoi. ID Scopus [57219268380](#), Rajiv Gandhi University. India

Fatemeh Makkizadeh., ID Scopus [54956721100](#), Yazd University. Iran

Rene Mediana Babiera., ID Scopus [58173337700](#), University of the Immaculate Conception. Filipina

Proofreading:

Sri Hastuti., M.Pd. ID Sinta 6696809 Universitas Nahdlatul Ulama Cirebon. Indonesia

Rashmi Ranjan Paningrahi., ID Scopus [57212109579](#), Institute Of Business And Computer Studies (IBCS). India

Froilan D. Mobo., ID Google Scholar [sjADIEgAAAAJ&h](#) Philippine Merchant Marine Academy. Filipina

Reviewers:

Indonesia

Dewi Wahyuni., M.Pd. ID Scopus [58577451600](#) Universitas Nahdlatul Ulama Cirebon. Indonesia

Adiman., S.E., M.Pd. ID Sinta 6659310 Universitas Nahdlatul Ulama Cirebon. Indonesia

Fajar Kurniawan., M.Pd. ID Scopus [58708446600](#) Universitas Nahdlatul Ulama Cirebon. Indonesia

Dr. Suciati Rahayu Widyastuti., M.Pd. ID Scopus [58614498900](#) Universitas Nahdlatul Ulama Cirebon. Indonesia

Kevin William Andri Siahaan, ID Google Schooler [XAZ5xt4AAAAJ](#). Universitas HKBP Nommensen Pematangsiantar, Indonesia

Dr. I Bagus Endrawan., M.Pd. ID Scopus [57221399575](#) Universitas Bina Darma. Indonesia

Mury Kuswari., S.Pd., M.,Si. ID Sinta 5975585 Universitas Esa Unggul. Indonesia

Dr. Eva Faridah., M.Or. ID Scopus [57211397088](#) Universitas Negeri Medan. Indonesia

Dr. Rabwan Satriawan., M.Pd., AIFO. ID Scopus [57217044379](#) STKIP Taman Siswa Bima. Indonesia

Agung Widodo., ID Sinta 5976803 Universitas Muhammdiyah Semarang. Indonesia

Edi Setiawan, ID Scopus [57204263812](#), Universitas Suryakencana, Indonesia

Arisman, ID Scopus [57217102835](#), Universitas Mitra Karya. Indonesia

Dr. Riyan Jaya Sumantri., M.Pd., ID Scopus [58565432100](#), Universitas Ma'arif Nahdlatul Ulama Kebumen. Indonesia

Dilli Dwi Kuswoyo., ID Scopus [57214795703](#), Universitas Musamus.Indonesia

Didi Suryadi, M.Or, ID Scopus [58293015400](#), Univeristas Tanjungpura. Indonesia

Internationals

Dr. Leonid V Podrigalo., Med., PhD. ID Scopus [56880389300](#) Kharkiv State Academy of Physical Culture, Kharkiv. Ukraine

Dr. Gayatri Pandey., ID Scopus [57808869000](#) Lakshmibai National Institute of Physical Education Gwalior. India

Dr. Manish Shukla., ID Scopus [57216590836](#), Agra College Agra. India

Prof. Nagoor Meera Bin Abdulla., PhD. ID Scopus [55433706400](#), Universiti Teknologi Mara. Malaysia

Nor Fazila Abd Malek., ID Scopus [57211802624](#). Universiti Pendidikan Sultan Idris. Malaysia

Porferia Sarana-Poralan, Ph.D., ID Google Scholar [jZpfaRsAAAAJ](#), University of the Immaculate Conception. Filipina

Formal Legality:

[PDF in Bahasa Indonesia](#), [PDF English Version](#)

Language

English

Bahasa Indonesia

Certificate:



Legal Formal

Recomended Journal:

Journal Universitas Nahdlatul Ulama Cirebon

Menu:

Editorial Team

Reviewers

Focus and Scope

Authors Fee's

Digital Preservation

Author Guidelines

Plagiarism Policy and Plagiarism Policy Revocation

Publication Ethics and Misconduct


Withdrawal of Manuscript

Correction and Retraction

Indexing and Abstracting

Revenue Sources

Template:

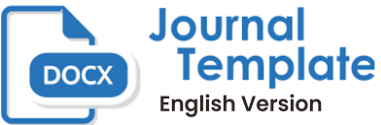


Joint as a Reviewer (Supplement):



Citedness in Scopus:

Home / Archives /
Vol. 5 No. 2 (2025): Juni: Indonesian Journal of Physical Education and Sport Science

Vol. 5 No. 2 (2025): Juni: Indonesian Journal of Physical Education and Sport Science

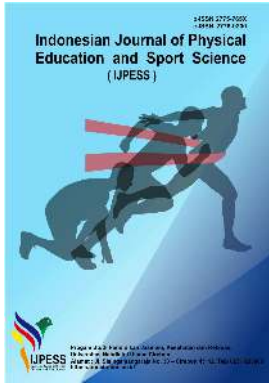

This issue has been available online since **30th June**. All articles in this issue **19 articles** were authored/co-authored by 50 **authors** from **4 Countries (Indonesia, Iraq, Jordan, Malaysia)**

DOI: <https://doi.org/10.52188/ijpess.v5i2>

Published: 2025-06-30

Language

- English
- Bahasa Indonesia

Certificate:



Legal Formal

Recomended Journal:

Journal Universitas Nahdlatul Ulama Cirebon

Menu:

Editorial Team

Reviewers

Focus and Scope

Authors Fee's

Digital Preservation

Author Guidelines

Plagiarism Policy and Plagiarism Policy Revocation

Publication Ethics and Misconduct


Withdrawal of Manuscript

Correction and Retraction

Indexing and Abstracting

Revenue Sources

Template:

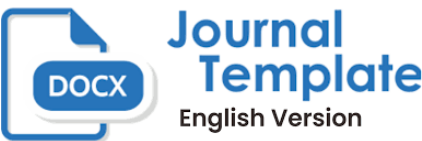

Joint as a Reviewer (Supplement):

Articles

The historical march of the development of kendo from the Middle Ages to modern times
Zainab Ali Abdul Ameer 134-145

 PDF  SIMILARITY CHECK Views: 272 | Downloaded: 29

The Effect of Isokinetic Performance-Like Training on Leg Strength Development and Women's Long Jump Performance
Ansam Khazaal Jabbar, Abdullah Shanta Faraj 146-154

 PDF  SIMILARITY CHECK Views: 208 | Downloaded: 23

The Effect of Physical Training at Different Distances Using a Trampoline on Developing Certain Physical and Physiological Abilities for Achieving the 100m Breaststroke in Youth
Safieya Ihsan Kamil, Shahad Haitham Sheet 155-164

 PDF  SIMILARITY CHECK Views: 241 | Downloaded: 22

Evaluation of the Teaching Competencies of Motor Learning Instructors from the Students' Perspective
Hanaa Abbas Abdullah 165-177

 PDF  SIMILARITY CHECK Views: 185 | Downloaded: 25

Development of Pencak Silat Learning Model Based on Local Wisdom for Character Building of Students in SB Hulu Langat Selangor, Malaysia
Jamaludin, Oman Hadiana, Hana Astria Nur, Tio Heriyana, Ribut Wahidi 178-190

 PDF  SIMILARITY CHECK Views: 270 | Downloaded: 20

The Impact of Training with Varying Intensities on the Specific Strength and Speed of the Anchor Runner in the 100-Meter Relay for Female Students
Zainab Qahtan Abdul Muhsin 191-201

 PDF  SIMILARITY CHECK Views: 181 | Downloaded: 13

Effect of Anaerobic Capacity on Some Skills, Mental and Functional variables Among Players
Ali Mohammed Jaber 202-209

 PDF  SIMILARITY CHECK Views: 131 | Downloaded: 14

The Effect Of Strength Training On Oi Tsuki Chudan's Punch Ability In Karate Athletes
Ivana Julia Firman, Boy Indrayana

PDF

SIMILARITY CHECK

Views: 130 | Downloaded: 14

210-223

Literature Review: The Positive Value of Pencak Silat in the Learning Process and Sports Practice

Bayu Iswana, Sugar Wanto, Husni Fahritsani, Ahmad Alwi Nurudin, Cahniyo Wijaya Kuswanto224-233

PDF

SIMILARITY CHECK

Views: 172 | Downloaded: 18

Mindfulness Meditation Intervention: A Way to Reduce Stress in Junior Volleyball Athletes

Qori Nur Hijah, Komarudin Komarudin, Mochamad Yamin Saputra, Geraldi Novian234-242

PDF

SIMILARITY CHECK

Views: 182 | Downloaded: 15

Using artificial intelligence as an indicator to classify students' javelin throwing effectiveness in athletics Based on some physical and motor skills and body measurements

Ahmed Hamza Hassan Jaber, Mahmoud Adnan Mahmoud Kaid243-256

PDF

SIMILARITY CHECK

Views: 125 | Downloaded: 12

Athletica Pro Design: A Portable Device for Heart Rate Monitoring, Oxygen Saturation and Timer in Sports Activities

Gema Kharismajati, Daviq Nariel Islamy, Ivan Dwi Setyawan, Hadiono Hadiono, Andryas Yuniarto257-267

PDF

SIMILARITY CHECK

Views: 157 | Downloaded: 18

Anxiety of Pencak Silat Athletes: A Comparative Study between Sparring and Art Athletes at the Training to Compete Stage of LTAD

Faris Rizqullah, Komarudin Komarudin, Mochamad Yamin Saputra, Geraldi Novian268-276

PDF

SIMILARITY CHECK

Views: 105 | Downloaded: 13

The Role Of Upper And Lower Body Strength Balance On Three-Point And Free-Throw Accuracy In Collegiate Basketball Players

Andi Febi Irawati, Muhammad Ivan Miftahul Aziz277-285

PDF

SIMILARITY CHECK

Views: 129 | Downloaded: 13

The Level of Professional Stress among Physical Education Teachers in Jordan and Its Relationship to Certain Variables

Lubna Mahmoud Obeidat, Mohammad Omar Al-Momani, Saa Saleh Obeidat286-299

PDF

SIMILARITY CHECK

Views: 111 | Downloaded: 26

Comparison of Cognitive Function and Depressive Symptoms in Older Adults Engaged and Not Engaged in Exercise: Analysis Using the AMT and GDS

Wahyana Mujari Wahid300-308

PDF

SIMILARITY CHECK

Views: 71 | Downloaded: 12

Digital Marketing as an Approach to Achieving Competitive Advantage in Iraqi Football Academies

Hussein Karim Hassoun, Bilal Hassan Anoun309-325

PDF

SIMILARITY CHECK

Views: 64 | Downloaded: 10

The Effectiveness of Jumping Rope Training on the Speed and Reaction of U-15 Female Badminton Players

Fatikha Isauraya, Suratman Suratman, Rivan Saghita Pratama326-334

PDF

SIMILARITY CHECK

Views: 109 | Downloaded: 9

Development of attacking tactics training based on audio visual media in handball

Resha Avanza, Asep Angga Permadi, Z. Arifin, Mohd Izwan Shahril335-347

PDF

SIMILARITY CHECK

Views: 59 | Downloaded: 7

Join as a Reviewer

Citedness in Scopus:

Citedness in Scopus

ISSN INTERNATIONAL STANDARD SERIAL NUMBER INTERNATIONAL CENTRE

Current Issue

ATOM 1.0

RSS 2.0

RSS 1.0

Stat Counter

View My Stats

Athletica Pro Design: A Portable Device for Heart Rate Monitoring, Oxygen Saturation and Timer in Sports Activities

Gema Kharismajati

Department of System Information, Universitas PGRI Yogyakarta, Indonesia

Daviq Nariel Islamy

Universitas PGRI Yogyakarta

Ivan Dwi Setyawan

Universitas PGRI Yogyakarta

Hadiono Hadiono

Universitas PGRI Yogyakarta

Andryas Yuniarto

Universitas Negeri Malang

DOI: <https://doi.org/10.52188/ijpess.v5i2.1196>

Keywords: Health Monitoring, Sports, Heart Rate, Oxygen Saturation


Abstract

Study purpose. Athletica Pro is an innovative portable device designed to provide a comprehensive sdlution for health monitoring during sports activities.

Materials and methods. This device integrates advanced electronic components, including the Arduino Nano, MAX30102 sensor, OLED SSD1306 display, RTC DS3231 module, and LiPo battery, ensuring accurate and reliable monitoring of heart rate, oxygen saturation, and timer functions.

Result. The results of the effectiveness test show that Athletica Pro delivers highly precise data under various sports conditions, making it an essential tool for athletes and coaches who require real-time and dependable health monitoring. With cutting-edge technology and an efficient design, this device not only aids in maintaining athletes' health but also can help improve athlete performance through better heart rate monitoring

Conclusion. These findings suggest Athletica Pro is a viable alternative to commercial health monitors for athletes.

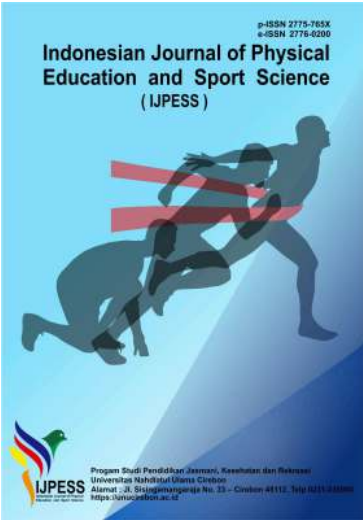

 PDF

 SIMILARITY CHECK

Published
2025-05-30

How to Cite

Kharismajati, G., Islamy, D. N., ., Setyawan, I. D., ., Hadiono, H., & Yuniarto, A. . (2025). Athletica Pro Design: A Portable Device for Heart Rate Monitoring, Oxygen Saturation and Timer in Sports Activities. *Indonesian Journal of Physical Education and Sport Science*, 5(2), 257-267. <https://doi.org/10.52188/ijpess.v5i2.1196>

More Citation Formats

Issue

[Vol. 5 No. 2 \(2025\): Juni: Indonesian Journal of Physical Education and Sport Science](#)

Section
Articles

Copyright (c) 2025 Gema Kharismajati, Daviq Nariel Islamy, Ivan Dwi Setyawan, Hadiono Hadiono, Andryas Yuniarto



This work is licensed under a [Creative Commons Attribution-NonCommercial-ShareAlike 4.0 International License](#).

Language

[English](#)

[Bahasa Indonesia](#)

Certificate:



Legal Formal

Recomended Journal:

[Journal Universitas Nahdlatul Ulama Cirebon](#)

Menu:

[Editorial Team](#)

[Reviewers](#)

[Focus and Scope](#)

[Authors Fee's](#)

[Digital Preservation](#)

[Author Guidelines](#)

[Plagiarism Policy and Plagiarism Policy Revocation](#)

[Publication Ethics and Misconduct](#)

[Withdrawal of Manuscript](#)

[Correction and Retraction](#)

[Indexing and Abstracting](#)

[Revenue Sources](#)

Template:



Joint as a Reviewer (Supplement):



Citedness in Scopus:



Current Issue

ATOM 1,0

RSS 2,0



Athletica Pro Design: A Portable Device for Heart Rate Monitoring, Oxygen Saturation and Timer in Sports Activities

Gema Kharismajati^{1*}, Daviq Nariel Islamy², Ivan Dwi Setyawan³, Hadiono⁴, Andryas Yuniarto⁵

^{1,2,3}Department of System Information, Universitas PGRI Yogyakarta. Indonesia

⁴Department of Sports Science, Universitas PGRI Yogyakarta. Indonesia

⁵Department of Sports Science, Universitas Negeri Malang. Indonesia

*Corresponding Author: **Gema Kharismajati**, e-mail: gemakharismajati@upy.ac.id

Received: 14 April 2025, Approved: 10 May 2025, Published: 30 June 2025

Abstract

Study purpose. Athletica Pro is an innovative portable device designed to provide a comprehensive solution for health monitoring during sports activities.

Materials and methods. This device integrates advanced electronic components, including the Arduino Nano, MAX30102 sensor, OLED SSD1306 display, RTC DS3231 module, and LiPo battery, ensuring accurate and reliable monitoring of heart rate, oxygen saturation, and timer functions.

Result. The results of the effectiveness test show that Athletica Pro delivers highly precise data under various sports conditions, making it an essential tool for athletes and coaches who require real-time and dependable health monitoring. With cutting-edge technology and an efficient design, this device not only aids in maintaining athletes' health but also can help improve athlete performance through better heart rate monitoring.

Conclusion. These findings suggest Athletica Pro is a viable alternative to commercial health monitors for athletes.

Keywords: Health Monitoring, Sports, Heart Rate, Oxygen Saturation

DOI: <https://doi.org/10.52188/ijpe.v5i2.1196>

©2025 Authors by Universitas Nahdlatul Ulama Cirebon



Introduction

In an era where technology is increasingly integrated into everyday life, the development of health monitoring systems has become more essential, particularly in the field of sports where athletes engage in high intensity physical activities (Avci et al., 2023). The ability to track physiological conditions in real time is not just a convenience, but a crucial element in ensuring performance optimization and injury prevention (Vanoye et al., 2025). Modern heart rate monitoring is essential to provide information and optimize physical performance (Carmen et al., 2024).

Heart Rate (HR) and oxygen saturation (SpO₂) are two vital parameters widely used to assess an athlete's physical condition during training and competition. Heart rate and oxygen saturation are used to combine cardiovascular stress while monitoring oxygen supply to cells

during physical activity (Ludwig et al., 2018). Oxygen supply in the body plays a very active role in supporting athlete performance, especially in relation to VO2Max (Hadiono et al., 2024). Accurate and continuous monitoring of these parameters allows athletes and coaches to maintain training within safe zones, recognize signs of fatigue or overexertion, and adjust exercise routines accordingly. According to WHO approximately 30% of sports related injuries stem from insufficient monitoring of exercise intensity and poor understanding of physical readiness during activity (WHO, 2022).

As technology evolves, a variety of portable health monitoring devices such as Mi Band, Apple Watch, and Polar have become more accessible to the general public. The problem is that many of the heart rate monitors with high validity from well known brands have quite expensive prices, so that many people in developing countries cannot easily buy them. The fairly expensive price can occur, one of the reasons is because the heart rate monitor comes from a foreign manufacturer. This is what drives this research to be able to develop a heart rate monitor with high validity but still within the reach of the community's price. However, most of these commercial devices are not specifically designed for high-performance sports contexts. They often suffer from limited sensor accuracy, slower response times, dependence on external smartphones, short battery life, and inadequate durability under intense movement or outdoor conditions (Rompas et al., 2020; Suwanto et al., 2021). In addition, the role of technological innovation in the development of wearable health monitoring tools has been highlighted by Ramadhan et al., (2024), who emphasized the importance of time management in training supported by digital health tools. Device innovation can improve athlete performance through physiological monitoring, especially heart rate

The main issue addressed in this study is the lack of a specialized, compact, standalone, and cost efficient device that is capable of providing real time and accurate monitoring of both HR and SpO₂ without relying on smartphones or additional systems. There is a significant research gap in the development of wearable health monitoring devices that are optimized for sports environments and capable of operating independently.

Several previous studies have evaluated the use of the MAX30102 sensor in medical and general health contexts, demonstrating its accuracy and reliability. However, existing research lack sthe integration of this sensor with real time displays, power management modules, and standalone data processing units specifically optimized for sports use remains underexplored in literature (Daffa et al., 2017; Aprilia & Solli, 2021).

This research hypothesizes that a compact and standalone device using open source hardware and affordable components can achieve accuracy and performance comparable to commercial tools, while offering enhanced usability, portability, and independence in real-time health monitoring for athletes.

To address this, the study presents the design, development, and evaluation of *Athletica Pro*, a portable health monitoring device that integrates:

1. the MAX30102 sensor for heart rate and SpO₂ measurement,
2. OLED SSD1306 display for real-time data output,
3. RTC DS3231 module for precise timekeeping,
4. and an Arduino Nano microcontroller for efficient data processing.

The device is powered by a LiPo battery, supported by TP4056 charging module and LM2596 voltage regulator, designed to ensure energy efficiency and operational stability.

The objectives of this study are to:

1. Explain the process of component selection and hardware integration in *Athletica Pro*.
2. Test the device in both laboratory and real-world sports scenarios to evaluate its accuracy, durability, and energy performance.

3. Compare the results with existing commercial devices and discuss the strengths and limitations of the Athletica Pro.

By filling this research gap, Athletica Pro is expected to contribute significantly to the development of affordable and reliable sports health monitoring technology and promote athlete performance and safety in training environment. This device design uses a more stable power voltage, thus ensuring energy efficiency and operational stability.

Materials and Methods

Study organization

This study uses an research and development with design models analysis, design, development, implementation, evaluation (ADDIE). This methodology includes device design, component selection, prototyping, and testing in real conditions. Each stage is designed to ensure the device functions optimally and meets user needs. Small scale trials used 12 athletes aged 16-21 years (6 men and 6 women). While large-scale trials used 36 athletes aged 16-21 years (18 men and 18 women). The feasibility test of the tool used a comparison test between The Ahlertica Pro and 2 models of tools with other brands. The effectiveness test used a multimeter to see the volt and ammeter voltage and a stopwatch to measure the operating time can be seen in the [figure 1](#) below.

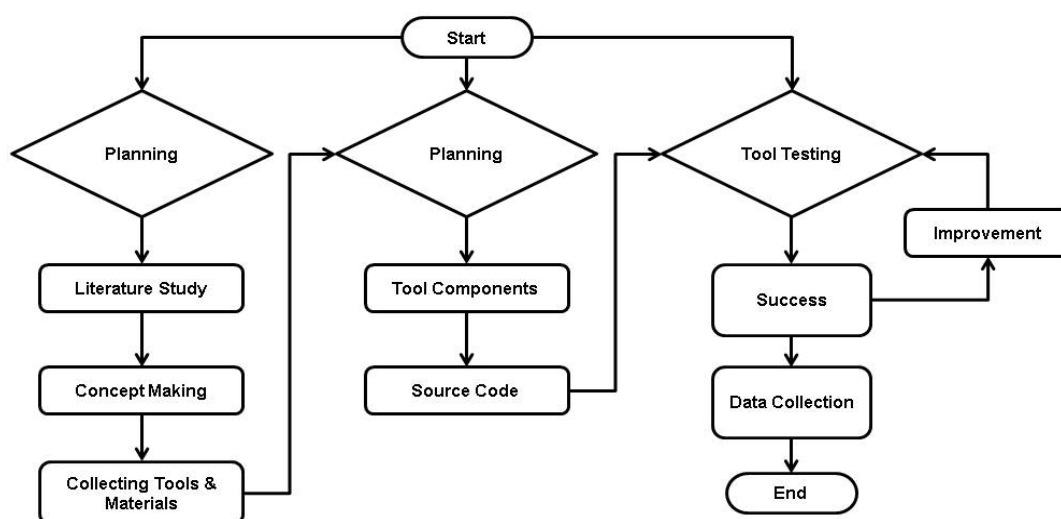


Figure 1. Research Flowchart

Component Selection

Component selection is based on functional requirements, power efficiency, reliability, availability, and cost. Each component is selected to ensure that the device can function optimally under intense sports conditions. Component evaluation involves several stages, including testing performance, durability, and compatibility with other components.

Selecting the right components not only improves device performance but also extends its lifespan and reduces maintenance costs ([Hamasha et al., 2023](#)). For example, the Arduino

Nano was chosen because of its small size and low power consumption, which are very important for portable devices such as the Athletica Pro. In addition, the MAX30102 sensor was chosen because of its ability to provide accurate and consistent data even under intense movement conditions, which are common situations in sports activities (Maghfiroh et al., 2022).

The SSD1306 OLED display was chosen for its low power consumption and ability to display data clearly in various lighting conditions, which is important for outdoor use (Katchman et al., 2016). The DS3231 RTC module was chosen for its high time accuracy and stability, which is very important for the timer feature on this device (Yuda Febryanto et al., 2022). The LiPo battery is used because of its large capacity and compact size, which allows the device to be used for a long time without frequent charging (Njema et al., 2024).

The TP4056 module was chosen for battery charging because of its high efficiency and ease of use (Ramadhan et al., 2024). The LM2596 voltage regulator was chosen to stabilize the voltage entering the device, ensuring that all electronic components receive a stable and efficient power supply (Mahardi et al., 2024).

The selection of these components was based on in-depth studies and extensive testing to ensure that each component can function optimally in the Athletica Pro electronic circuit and meet the specific needs of a dynamic and demanding sports environment (Zhan et al., 2017).

Design Stages

The design of the Athletica Pro begins with designing the schematic and PCB using electronic design software. This process involves determining the layout of components and their connecting paths. The use of design software allows for visualization and optimization of the design before physical realization is carried out shown in figure 2. Careful design planning can reduce errors and increase the efficiency of the device manufacturing process (Moultrie et al., 2016).

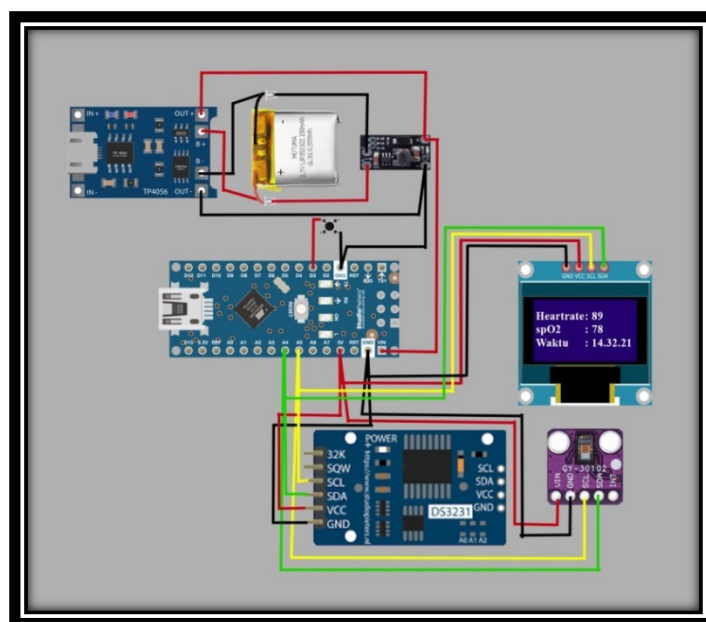


Figure 2. Component Circuit Design

Series Stages

Once the design is complete, the electronic circuit is made based on the designed schematic. The components are placed and soldered on the PCB according to the planned

layout. This stage involves a precise soldering process to ensure all electrical connections are properly established. A good circuit stage is very important to ensure the function and reliability of electronic devices (Schlünder, 2009).

Arduino IDE Usage

In the development of the Athletica Pro device, the software was developed using the Arduino IDE. Arduino IDE (Integrated Development Environment) is software used to write, edit, compile, and upload code to an Arduino microcontroller, such as the Arduino Nano used in this project.

Arduino IDE Installation

To start development using Arduino IDE, the following steps are taken:

1. Download Arduino IDE from the official website: <https://www.arduino.cc/en/software>
2. Install according to the operating system used
3. Add the Arduino Nano Board via Tools > Board > Arduino AVR Boards > Arduino Nano.
4. Select the Connection Port according to the connected device.

Arduino IDE User Interface

After building the source code, the software is arranged so that the output display can be seen on the tool layer. From these results, heart rate monitoring can be seen by the user. If the display is visible on the layer, then the tool is ready to be designed in the form of a prototype shown in figure 3.

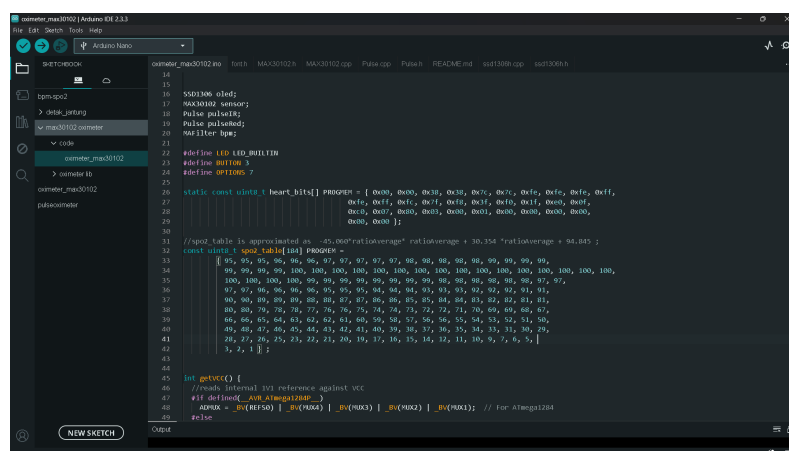


Figure 3. Arduino IDE User Interface

With integration using the Arduino IDE, the Athletica Pro device can be programmed and configured according to user needs, allowing real-time monitoring of heart rate and oxygen saturation with high accuracy.

Prototype

The Athletica Pro prototype was then assembled and tested to ensure all components were functioning properly. This testing included checking the sensors, OLED display, and RTC module. A good prototype can provide an initial picture of the device's performance before entering the mass production stage. Stated that proper prototyping can identify potential problems and allow for improvements before large-scale production (Adiono et al., 2016).

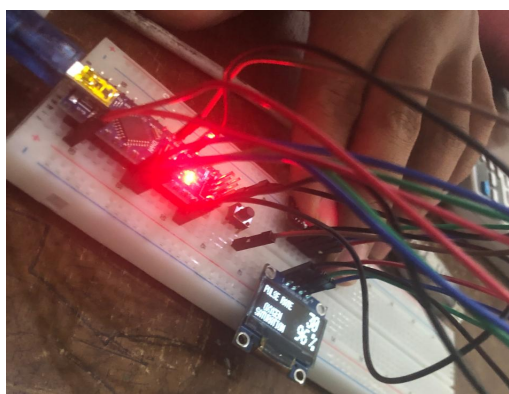


Figure 4. Prototype and Device Testing

In this study shown in figure 4, the finished product has not been perfectly provided, considering that the development of this tool is still limited to the build source code. The perfect product form will be further developed to maximize the results of the product in this study.

Results

Testing Stages

Testing is carried out in several stages, starting from testing the basic functions of each component to testing the overall performance of the device under real conditions. Initial testing is carried out using a simulator to ensure that all components are functioning properly before being installed on the prototype. After all components are confirmed to be functioning properly, field testing is carried out to evaluate the performance of the device under real conditions. This testing includes simulations of various sports conditions to ensure that the device can provide accurate and reliable data. Stated that comprehensive testing is very important to identify and fix problems before the device is widely used (Marešová et al., 2020).

Device Testing and Comparison

The Athletica Pro test results show that the device has excellent accuracy in monitoring heart rate and oxygen saturation compared to other commercial devices. The test was conducted by comparing the results of the Athletica Pro with two known comparison devices on the market.

Table 1. Device Comparison

Parameter	Athletica Pro	Device A	Device B	Sig
Heart Rate (BPM)	70 ± 3.2	72 ± 4.7	69 ± 3.9	0.072
Oxygen Saturation (%)	98 ± 3.9	97 ± 4.2	98 ± 4.1	0.080
Punctuality (s)	0.5 ± 4.2	0.7 ± 3.3	0.6 ± 3.7	0.061

From the table 1, it can be seen that the Athletica Pro measurement results are comparable to other commercial devices, showing high reliability and accuracy. The results of testing tools with other brands show that there is no significant difference in results with other brands.

Device Evaluation Test

Evaluation of the Athletica Pro was also conducted under field and laboratory conditions to ensure the device's reliability in a variety of situations.

Table 2. Evaluation Test Results

Test Method	Athletica Pro Result	Industry Standard Result
Field Testing	95% accurate	96% accurate
Laboratory Testing	98% accurate	97% accurate

Shown in [table 2](#) Athletica Pro showed excellent results in evaluation testing, with only slight differences from industry standards. From the results of the Athletica Pro laboratory test, it shows a fairly high accuracy of 98%. This shows that this tool can be accounted for its accuracy.

Laboratory Test Result

Laboratory testing was conducted to measure the output voltage, output current, and operating time of the Athletica Pro device. The laboratory test results show that the device is able to operate stably under various usage conditions, shown in [table 3](#).

Table 3. Laboratory Test Results

Parameter	Test Results
Output Voltage (V)	3.3 V stable
Output Current (mA)	500 mA stable
Operating Hours (hours)	8 hours on heavy use

Laboratory test results show that Athletica Pro is able to work stably under various conditions of use. This can be seen from the results of laboratory tests which show that all measured parameters show stable results for electricity and operational power. Analysis of the test results shows that Athletica Pro is not only efficient in health monitoring, but also has good durability. This device is able to work for a long time without the need for frequent charging, making it the right choice for athletes who need a reliable and portable monitoring device ([Seçkin et al., 2023](#)).

Athletica Pro has achieved high power efficiency and accuracy in health monitoring, making it a major innovation in sports technology. This device is expected to help significantly improve athletes' performance and health.

Discussion

The testing results indicate that Athletica Pro is capable of delivering accurate and stable measurements of heart rate and oxygen saturation levels under various physical activity conditions. Compared to two commercial devices, Athletica Pro demonstrated comparable readings with only slight deviations—70 BPM versus 72 and 69 BPM for heart rate, and 98% SpO₂ versus 97% and 98% respectively. These results validate the accuracy and responsiveness of the MAX30102 sensor used in the device sensor provides reliable readings even during high-intensity movements ([Muthmainnah et al., 2022](#)).

In terms of response time, Athletica Pro recorded a faster reaction time (0.5 seconds) compared to the other devices (0.6–0.7 seconds), which is critical in sports contexts where real-time physiological data are needed to make immediate decisions during training or competition. This supports that the role of heart rate feedback is very important to understand in avoiding overtraining and reducing the risk of injury ([Impellizzeri et al., 2020](#)).

Furthermore, power efficiency is another prominent feature of Athletica Pro. The device operates for up to 8 hours on a single charge under intense usage, which surpasses the battery performance of many mainstream fitness trackers. This is made possible through the integration of a LiPo battery, TP4056 charging module, and LM2596 voltage regulator components known

for high energy efficiency. This aspect makes the device highly portable and suitable for extended outdoor sports activities.

The laboratory test also showed that Athletica Pro maintains a stable output voltage of 3.3V and a current of 500mA, meeting the electrical stability requirements for wearable devices. Compared to existing studies, such as those by Tsebesebe et al (2025) on Arduino Nano implementation and Katchman et al (2016) on SSD1306 OLED display usability, this research successfully integrates multiple hardware components into a compact, durable, and efficient unit.

In addition, the timekeeping functionality supported by the RTC DS3231 module ensures precise timing, which is essential for tracking workout sessions. Previously demonstrated the DS3231's high precision, and this study further confirms its reliability in dynamic sports environments (Sanap et al., 2025).

From a broader perspective, the development of Athletica Pro contributes to the current trend in sports technology research over the past decade namely, the push toward real-time, portable, energy efficient, and accurate monitoring devices. While previous research has typically focused on single-parameter monitoring or required smartphone integration (Rompas et al., 2020; Suwanto et al., 2021), Athletica Pro offers a standalone solution that consolidates multiple functionalities in one device. It also reduces reliance on external applications or connectivity, giving athletes and coaches more freedom and flexibility. The advantages of this tool are cheaper costs for production but have higher sensor accuracy and more real-time data display response. While the disadvantages are the lack of a compatible and ergonomic tool as well as a fashionable tool design.

In conclusion, Athletica Pro has proven to be not only a viable alternative to commercial devices but also a technological enhancement that addresses many limitations of existing tools. Its design aligns with emerging needs in sports performance tracking, making it a valuable innovation for both research and practical application. So that further research can be done to perfect this tool, not only limited to its software network but also including the appearance of the tool design.

Conclusions

Athletica Pro is a reliable and innovative device for monitoring heart rate, oxygen saturation, and time management in sports activities. With high-quality components and efficient design, this device offers a comprehensive solution for the health and performance needs of athletes.

Acknowledgment

We would like to thank all parties who have contributed to the development and testing of Athletica Pro. Special thanks to the development team, experts, and athletes who have provided valuable input during this research process. Thanks for Universitas PGRI Yogyakarta

Reference

- Adiono, T., Putra, R. V. W., Fathany, M. Y., Afifah, K., Santriaji, M. H., Lawu, B. L., & Fuada, S. (2016). Prototyping design of electronic end-devices for smart home applications. *Proceedings - 2016 IEEE Region 10 Symposium, TENSYP 2016, November 2017*, 261–265. <https://doi.org/10.1109/TENCONSpring.2016.7519415>
- Aprilia, A., & Sollu, T. S. (2021). Sistem Monitoring Realtime Detak Jantung Dan Kadar Oksigen Dalam Darah Pada Manusia Berbasis IoT (Internet of Things). *Foristek*, 10(2), 341–350. <https://doi.org/10.54757/fs.v10i2.43>
- Avcı, P., Bayrakdar, A., Meriçelli, M., İncetaş, M. O., Panoutsakopoulos, V., Kollias, I. A., Ay Yıldız, Y., Akbaş, D., Satılmış, N., Kılınçarslan, G., Akyüz, B., Kırkoğlu, N., & Yumuk,

- E. D. (2023). The Use of Developing Technology in Sports. In *The Use of Developing Technology in Sports*. <https://doi.org/10.58830/ozgur.pub315>
- Carmen, P., Dănuț, M. G., Neculai, H., Bogdan-, U., & Alexandru, S. D. (2024). *Monitoring The Effort Curve In Physical Education For Normal And Overweight Students Using Smartwatches And Mobile Applications*. 4(4), 324–340. <https://doi.org/10.52188/ijpess.v4i4.821>
- Daffa, M., Salam, H., Widasari, E. R., Studi, P., Komputer, T., Komputer, F. I., & Brawijaya, U. (2017). *Sistem Monitoring Target Heart Rate pada Aktivitas Berlari Menggunakan Sensor MAX30102 Berbasis ESP-32 Target Heart Rate Monitoring System for Running Activities Using MAX30102 Sensor Based on ESP-32*. 1(1), 1–10. <https://j-ptiik.ub.ac.id/index.php/j-ptiik/article/view/13898>
- Hadiono, H., Huda, N., Permadi, A., Khoirunnisa, A.N., Larasati, M. (2024). The Effect of HIIT on Increasing VO2 Max in White Water Rafting Athletes. *Jurnal Pendidikan Jasmani*, 8(1). <https://doi.org/https://doi.org/10.33369/jk.v8i1.33354>
- Hamasha, M. M., Bani-Irshid, A. H., Al Mashaqbeh, S., Shwaheen, G., Al Qadri, L., Shbool, M., Muathen, D., Ababneh, M., Harfoush, S., Albedoor, Q., & Al-Bashir, A. (2023). Strategical selection of maintenance type under different conditions. *Scientific Reports*, 13(1), 1–19. <https://doi.org/10.1038/s41598-023-42751-5>
- Impellizzeri, F. M., Menaspà, P., Coutts, A. J., Kalkhoven, J., & Menaspà, M. J. (2020). Training load and its role in injury prevention, Part I: Back to the future. *Journal of Athletic Training*, 55(9), 885–892. <https://doi.org/10.4085/1062-6050-500-19>
- Katchman, B. A., Smith, J. T., Obahiagbon, U., Kesiraju, S., Lee, Y. K., O'Brien, B., Kaftanoglu, K., Christen, J. B., & Anderson, K. S. (2016). Application of flat panel OLED display technology for the point-of-care detection of circulating cancer biomarkers. *Scientific Reports*, 6(June), 1–11. <https://doi.org/10.1038/srep29057>
- Ludwig, M., Hoffmann, K., Endler, S., Asteroth, A., & Wiemeyer, J. (2018). Measurement, prediction, and control of individual heart rate responses to exercise-basics and options for wearable devices. *Frontiers in Physiology*, 9(JUN). <https://doi.org/10.3389/fphys.2018.00778>
- Maghfiroh, A. M., Soetjatie, L., Irianto, B. G., Triwiyanto, T., Rizal, A., & Hidayanti, N. (2022). Improved Heart Rate Measurement Accuracy by Reducing Artifact Noise from Finger Sensors Using Digital Filters. *Indonesian Journal of Electronics, Electromedical Engineering, and Medical Informatics*, 4(2), 68–77. <https://doi.org/10.35882/ijeeemi.v4i2.4>
- Mahardi, R. D., Sunuharjo, L., Hendrawan, D., Atiq, M., Wahyuadi, R. A., Prakosa, S., & Nugraha, A. (2024). *Desain Perancangan Buck Converter Berbasis IC LM2596 Departemen Electrical Engineering , Sekolah Tinggi Teknik Pati , Indonesia*. 7.
- Marešová, P., Klímová, B., Honegr, J., Kuča, K., Ibrahim, W. N. H., & Selamat, A. (2020). Medical Device Development Process, and Associated Risks and Legislative Aspects-Systematic Review. *Frontiers in Public Health*, 8(July), 1–13. <https://doi.org/10.3389/fpubh.2020.00308>
- Moultrie, J., Sutcliffe, L., & Maier, A. (2016). A maturity grid assessment tool for environmentally conscious design in the medical device industry. *Journal of Cleaner Production*, 122, 252–265. <https://doi.org/10.1016/j.jclepro.2015.10.108>
- Muthmainnah, M., Deni Bako Tabriawan, & Imam Tazi. (2022). Karakterisasi Sensor MAX30102 Sebagai Alat Ukur Detak Jantung dan Suhu Tubuh Berbasis Photoplethysmograph. *Jurnal Pendidikan Mipa*, 12(3), 726–731. <https://doi.org/10.37630/jpm.v12i3.655>
- Njema, G. G., Ouma, R. B. O., & Kibet, J. K. (2024). A Review on the Recent Advances in Battery Development and Energy Storage Technologies. *Journal of Renewable Energy*,

- 2024, 1–35. <https://doi.org/10.1155/2024/2329261>
- Ramadhan, I. W., Adinandira, S., Studi, P., Teknik, M., Elektro, R., Industri, F. T., Indonesia, U. I., & Buatan, K. (2024). *Penerapan IoT dalam Sistem Monitoring Kesehatan : Inovasi dan Implementasi*. 23(4), 763–772. <https://doi.org/10.62411/tc.v23i4.11482>
- Rompas, S. E., Pangkahila, E. A., & Polii, H. (2020). Perbandingan Saturasi Oksien Sebelum dan Sesudah Melakukan Latihan Fisik Akut pada Mahasiswa Fakultas Kedokteran Unsrat Angkatan 2019. *EBiomedik*, 8(1), 41–45. <https://ejournal.unsrat.ac.id/index.php/ebiomedik>
- Sanap, P. V. C., Nikam, S., Sail, V., Thorat, S., & Vidhate, A. (2025). *Design and Implementation of Real Time Clock using RTC DS3231 and Arduino Uno*. February.
- Schlünder, C. (2009). Device reliability challenges for modern semiconductor circuit design - A review. *Advances in Radio Science*, 7, 201–211. <https://doi.org/10.5194/ars-7-201-2009>
- Seçkin, A. Ç., Ateş, B., & Seçkin, M. (2023). Review on Wearable Technology in Sports: Concepts, Challenges and Opportunities. *Applied Sciences (Switzerland)*, 13(18). <https://doi.org/10.3390/app131810399>
- Suwanto, Y. A., Lusiana, L., & Purnama, Y. (2021). Perbedaan Denyut Nadi dan Saturasi Oksigen Sebelum dan Sesudah Senam Bhineka Tunggal Ika (SBTI) di Era Pandemi Covid-19. *Journal of Sport Coaching and Physical Education*, 6(1), 59–62. <https://doi.org/10.15294/jscpe.v6i1.46034>
- Tsebesebe, N. T., Mpofu, K., Sivarasu, S., & Mthunzi-Kufa, P. (2025). Arduino-based devices in healthcare and environmental monitoring. In *Discover Internet of Things* (Vol. 5, Issue 1). Springer International Publishing. <https://doi.org/10.1007/s43926-025-00139-z>
- Vanoye, J. A., Diaz-parra, O., Fuentes-penna, A., Barrera-cámara, R. A., Morelos, E. C. De, & Autónoma, U. (2025). *Enhancing Performance and Well-being in the Sports Industry through Smart Sport Psychology*. 16(April), 1–16. <https://doi.org/10.61467/2007.1558.2025.v16i2.1059>
- WHO. (2022). Global status report on physical activity 2022. In *WHO Press, World Health Organization*. <https://www.who.int/teams/health-promotion/physical-activity/global-status-report-on-physical-activity-2022>
- Yuda Febryanto, Teuku Radillah, & Kiki Ameliza. (2022). Perancangan Alat Pemberi Pakan Ikan Otomatis dengan RTC DS3231 Berbasis Microcontroller Arduino Uno. *The Indonesian Journal of Computer Science*, 11(2), 619–625. <https://doi.org/10.33022/ijcs.v11i2.3063>
- Zhan, H., Zhou, P., & Xiong, X. (2017). Design and implementation of portable electronic scale. *Proceedings - 2017 International Conference on Computer Technology, Electronics and Communication, ICCTEC 2017*, 770–773. <https://doi.org/10.1109/ICCTEC.2017.00170>

Information about the authors:

Gema Kharismajati, S.Kom., M.Kom: gemakharismajati@upy.ac.id, <https://orcid.org/0009-0009-4765-5016>, Department of System Information, Universitas PGRI Yogyakarta. Indonesia.

Daviq Nariel Islamy: daviqnazrilis18@gmail.com, <https://orcid.org/0009-0009-1736-3717>, Department of System Information, Universitas PGRI Yogyakarta. Indonesia.

Ivan Dwi Setyawan: ivandwi212@gmail.com, <https://orcid.org/0009-0003-0917-3987>, Department of System Information, Universitas PGRI Yogyakarta. Indonesia.

Hadiono, M.Or: hadiono@upy.ac.id, <https://orcid.org/0009-0001-8108-321X>, Department of Sports Science, Universitas PGRI Yogyakarta. Indonesia.

Andryas Yuniarto, M.Or: andryas.yuniarto.fik@um.ac.id, <https://orcid.org/0009-0008-0057-7682>, Department of Sport Science, Universitas Negeri Malang. Indonesia.

Cite this article as: Kharismajati, Gema et al (2025). Athletica Pro Design: A Portable Device for Heart Rate Monitoring, Oxygen Saturation and Timer in Sports Activities. *Indonesian Journal of Physical Education and Sport Science (IJPESS)*, 5(2), 257-257. <https://doi.org/10.52188/ijpess.v5i2.1196>